

Certificate of Analysis

Nova Cell Peptides
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)

Sample Identification

Sample Name Bacteriostatic Water 3 mL
Batch Number 12-2028
Date Published 2026-07-23 12:35

Results for LIQ-0037

Stabilizers	Result	Unit	Uncertainty	Acceptable Range
Benzyl Alcohol Content Benzyl alcohol	0.93	%	[± 0.02]	0.9 - 1.1
Peptides	Result	Unit	Uncertainty	Acceptable Range
pH Determination pH determination	6.5		[± 0.1]	4.45 - 7
Microbiology	Result	Unit	Uncertainty	Acceptable Range
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.101	EU/vial	[± 0.002]	<= 0.25





Analysis Report




Sample Information


Injection Volume : 1
Data File : LIQ-0037_002.lcd
Method File : Benzylalcohol v2.0.lcm
Date Acquired : 21.07.2026 19:08:20

Chromatogram

uV

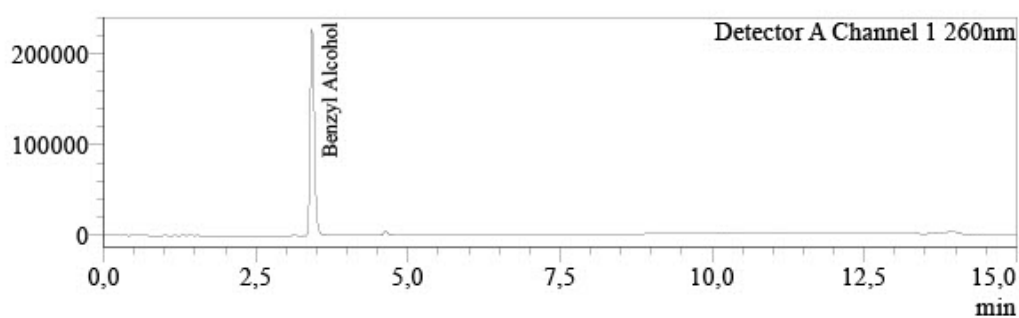

uV

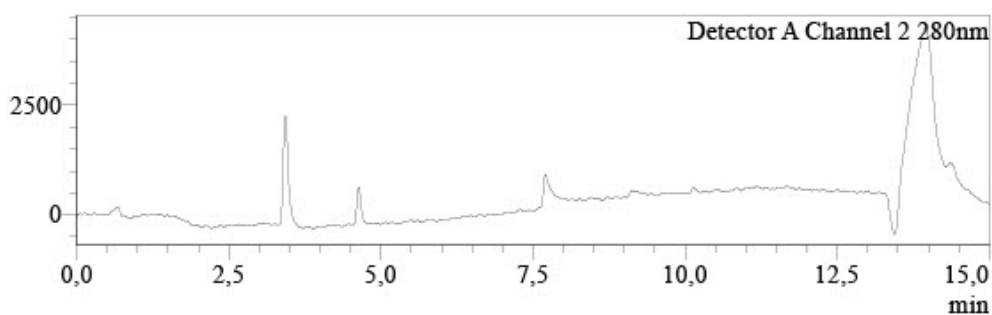

Peak Table

Detector A Channel 1 260nm

Peak#	Name	Ret. Time	Conc.	Unit	Area%
1	Benzyl Alcohol	3.423	0.928	% (m/m)	100.000
Total					100.000

Peak Table

Detector A Channel 2 280nm

Peak#	Name	Ret. Time	Conc.	Unit
Total				

Endotoxin Determination Report




File Information

Filename: C:\UVVis-Data\Data\File_260720_124259.vqud
Date/Time: 07/20/2026 12:42:33 PM

Instrument Information

Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

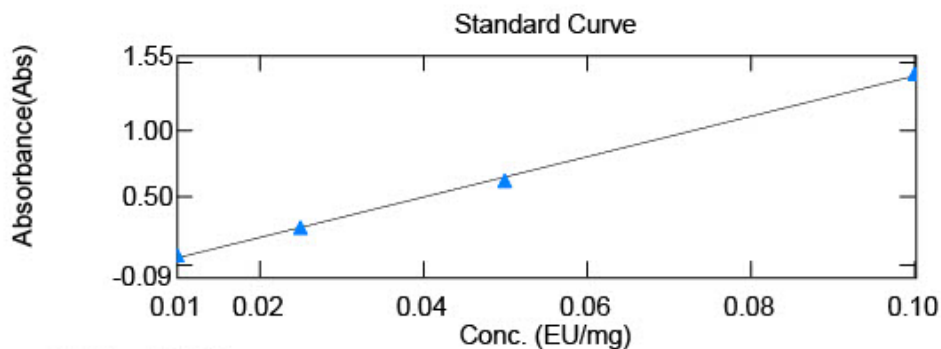

$$y = 15.0474x - 0.104044$$
$$r^2 = 0.99891$$

	Sample Name	Conc	Result	Dilution Rate
1	LYO-0363	0.267	0.097	20.00
2	LYO-0364	3.062	2.199	20.00
3	LYO-0365	2.603	1.855	20.00
4	LYO-0366	0.702	0.424	20.00
5	LYO-0367	3.216	2.315	20.00
6	LYO-0368	0.487	0.263	20.00
7	LYO-0369	0.422	0.213	20.00
8	LYO-0371	0.226	0.066	20.00
9	LYO-0372	0.243	0.079	20.00
10	LYO-0373	0.422	0.023	50.00
11	LYO-0374	0.303	0.124	20.00
12	LYO-0375	3.200	2.304	20.00
13	LYO-0376	0.664	0.395	20.00
14	LIQ-0037	0.101	0.048	10.00
15	LYO-0378	1.528	1.045	20.00

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.