

Certificate of Analysis



Nova Cell Peptides
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)


Sample Identification

Sample Name Retatrutide 10 mg
Batch Number N3-042603
Date Published 2026-08-19 16:20

Results for LYO-0586

Microbiology	Result	Unit	Uncertainty	Acceptable Range
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.068	EU/mg	[± 0.001]	



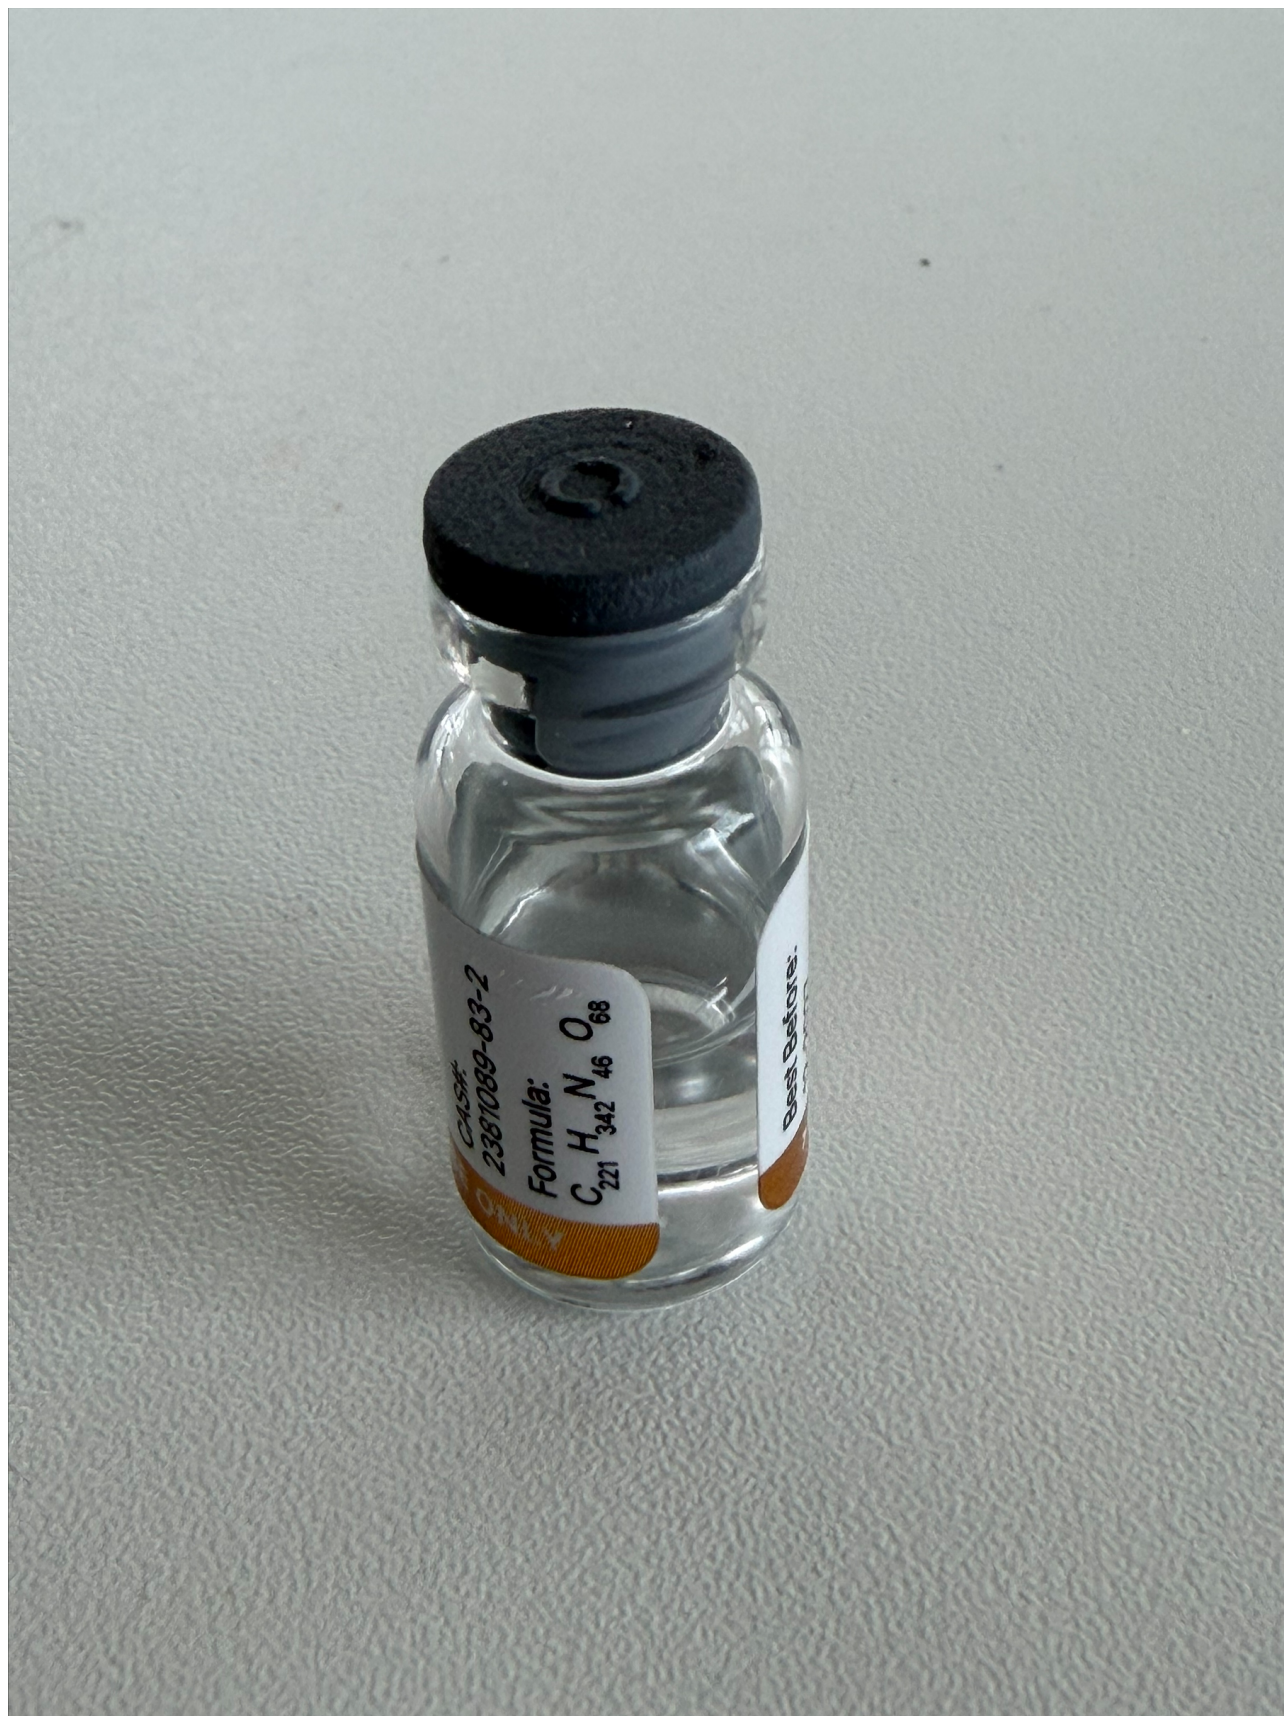

Endotoxin Determination Report




File Information

Filename: C:\UVVis-Data\Data\File_260813_140812.vqud
Date/Time: 08/13/2026 03:25:51 PM

Instrument Information

Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

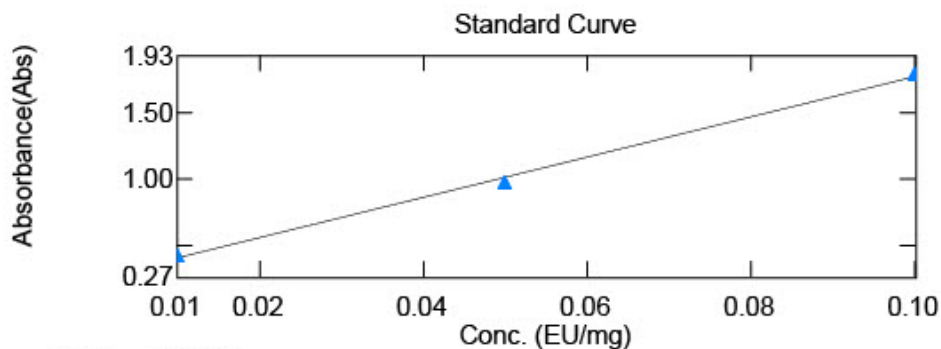

$$y = 15.1410x + 0.259749$$
$$r^2 = 0.99749$$

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
1	LYO-0573	0.816	0.8775	20.00
2	LYO-0560	0.765	0.8388	20.00
3	LYO-0559	1.047	1.0521	20.00
4	LYO-0583	3.016	1.4015	40.00
5	LYO-0584	1.016	1.0292	20.00
6	LYO-0586	0.678	0.7727	20.00
7	LYO-0588	-0.017	0.2472	20.00
8	LYO-0590	5.611	2.3837	40.00
9	LYO-0592	0.381	0.5482	20.00
10	LYO-0594	0.777	0.8479	20.00
11	LYO0595	1.338	1.2730	20.00
12	LYO-0596	1.397	0.7887	40.00
13	LYO-0597	0.634	0.4998	40.00
14	LYO-0598	1.159	1.1370	20.00
15	LYO-0599	0.486	0.6277	20.00
16	LYO-0546	-0.002	0.2587	30.00
17	LIQ-0051	-0.003	0.2210	1.00

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.