# Certificate of Analysis

LIQUILABS
Analytical services

**Nova Cell Peptides**
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

**Liquilabs s.r.o.**
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz

Verify Results Online

## Sample Identification

| | |
|---|---|
| **Sample Name** | Retatrutide 20 mg |
| **Batch Number** | N3-082604 |
| **Date Published** | 2026-09-09 14:35 |

## Results for LYO-0816

| Microbiology | Result | Unit | Uncertainty | Acceptable Range |
|---|---|---|---|---|
| Bacterial Endotoxin Chromgenic<br>USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test | 0.009 | *EU/mg* | [± 0] | |

**Liquilabs s.r.o.** • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

**Liquilabs s.r.o.** • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

# Endotoxin Determination Report

File Information
Filename: C:\UVVis-Data\Data\File_260908_140209.vqud
Date/Time: 09/08/2026 02:49:05 PM

Instrument Information
Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

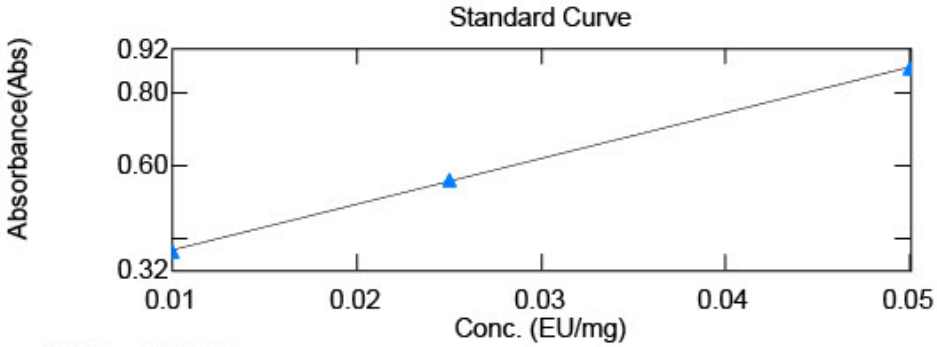


y = 12.4756 x + 0.244725
r2 = 0.99983

| | Sample Name | Conc | Raw_WL545.0 | Dilution Rate |
|---|---|---|---|---|
| 1 | LYO-0796 | 1.165 | 0.6079 | 40.00 |
| 2 | LYO-0797 | -0.177 | 0.1345 | 20.00 |
| 3 | LYO-0798 | 4.918 | 0.8582 | 100.00 |
| 4 | LYO-0799 | 0.017 | 0.2555 | 20.00 |
| 5 | LYO-0800 | -0.240 | 0.0947 | 20.00 |
| 6 | LYO-0801 | -0.278 | 0.0715 | 20.00 |
| 7 | LYO-0802 | 5.386 | 0.5807 | 200.00 |
| 8 | LYO-0803 | -0.250 | 0.0888 | 20.00 |
| 9 | LYO-0804 | 1.360 | 0.6688 | 40.00 |
| 10 | LYO-0805 | -0.253 | 0.0872 | 20.00 |
| 11 | LYO-0806 | -0.241 | 0.0945 | 20.00 |
| 12 | LYO-0807 | 0.052 | 0.2775 | 20.00 |
| 13 | LYO-0816 | -0.137 | 0.1591 | 20.00 |
| 14 | LYO-0818 | -0.155 | 0.1483 | 20.00 |
| 15 | LYO-0820 | -0.257 | 0.0843 | 20.00 |
| 16 | LYO-0822 | -0.283 | 0.0679 | 20.00 |
| 17 | LYO-0824 | -0.979 | 0.1226 | 100.00 |
| 18 | LYO-0832 | 2.564 | 0.5646 | 100.00 |
| 19 | LYO-0833 | -0.181 | 0.1320 | 20.00 |
| 20 | LYO-0834 | 0.248 | 0.3992 | 20.00 |



**Liquilabs s.r.o.** • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

| | Sample Name | Conc | Raw_WL545.0 | Dilution Rate |
|---|---|---|---|---|
| 21 | LYO-0835 | -0.209 | 0.1142 | 20.00 |
| 22 | LYO-0836 | 0.030 | 0.2636 | 20.00 |
| 23 | LIQ-0067 | -0.012 | 0.0947 | 1.00 |



**Liquilabs s.r.o.** • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

**Responsibles**

**Mr. Ján Galbavý**
*CEO*

Analysis results relate only to the samples tested.
This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.



**Liquilabs s.r.o.** • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz