

Certificate of Analysis



Nova Cell Peptides
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)

Sample Identification

Sample Name Retatrutide 10 mg
Batch Number N3-082604
Date Published 2026-09-09 14:35

Results for LYO-0818

Microbiology	Result	Unit	Uncertainty	Acceptable Range
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.017	EU/mg	[± 0]	





Endotoxin Determination Report




File Information

Filename: C:\UVVis-Data\Data\File_260908_140209.vqud
Date/Time: 09/08/2026 02:49:05 PM

Instrument Information

Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

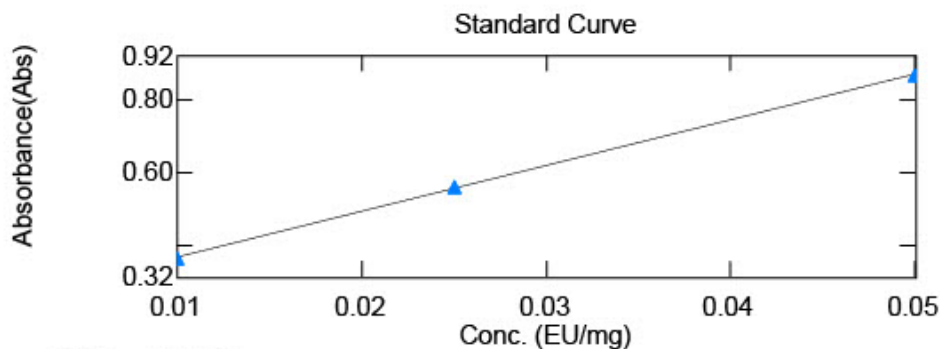

$$y = 12.4756x + 0.244725$$
$$r^2 = 0.99983$$

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
1	LYO-0796	1.165	0.6079	40.00
2	LYO-0797	-0.177	0.1345	20.00
3	LYO-0798	4.918	0.8582	100.00
4	LYO-0799	0.017	0.2555	20.00
5	LYO-0800	-0.240	0.0947	20.00
6	LYO-0801	-0.278	0.0715	20.00
7	LYO-0802	5.386	0.5807	200.00
8	LYO-0803	-0.250	0.0888	20.00
9	LYO-0804	1.360	0.6688	40.00
10	LYO-0805	-0.253	0.0872	20.00
11	LYO-0806	-0.241	0.0945	20.00
12	LYO-0807	0.052	0.2775	20.00
13	LYO-0816	-0.137	0.1591	20.00
14	LYO-0818	-0.155	0.1483	20.00
15	LYO-0820	-0.257	0.0843	20.00
16	LYO-0822	-0.283	0.0679	20.00
17	LYO-0824	-0.979	0.1226	100.00
18	LYO-0832	2.564	0.5646	100.00
19	LYO-0833	-0.181	0.1320	20.00
20	LYO-0834	0.248	0.3992	20.00

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
21	LYO-0835	-0.209	0.1142	20.00
22	LYO-0836	0.030	0.2636	20.00
23	LIQ-0067	-0.012	0.0947	1.00

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.