

Certificate of Analysis



Nova Cell Peptides
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)


Sample Identification

Sample Name GHK-Cu 50 mg
Batch Number Cu-082604
Date Published 2026-09-29 14:48

Results for LYO-0984

Microbiology	Result	Unit	Uncertainty	Acceptable Range
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.002	EU/mg	[± 0]	



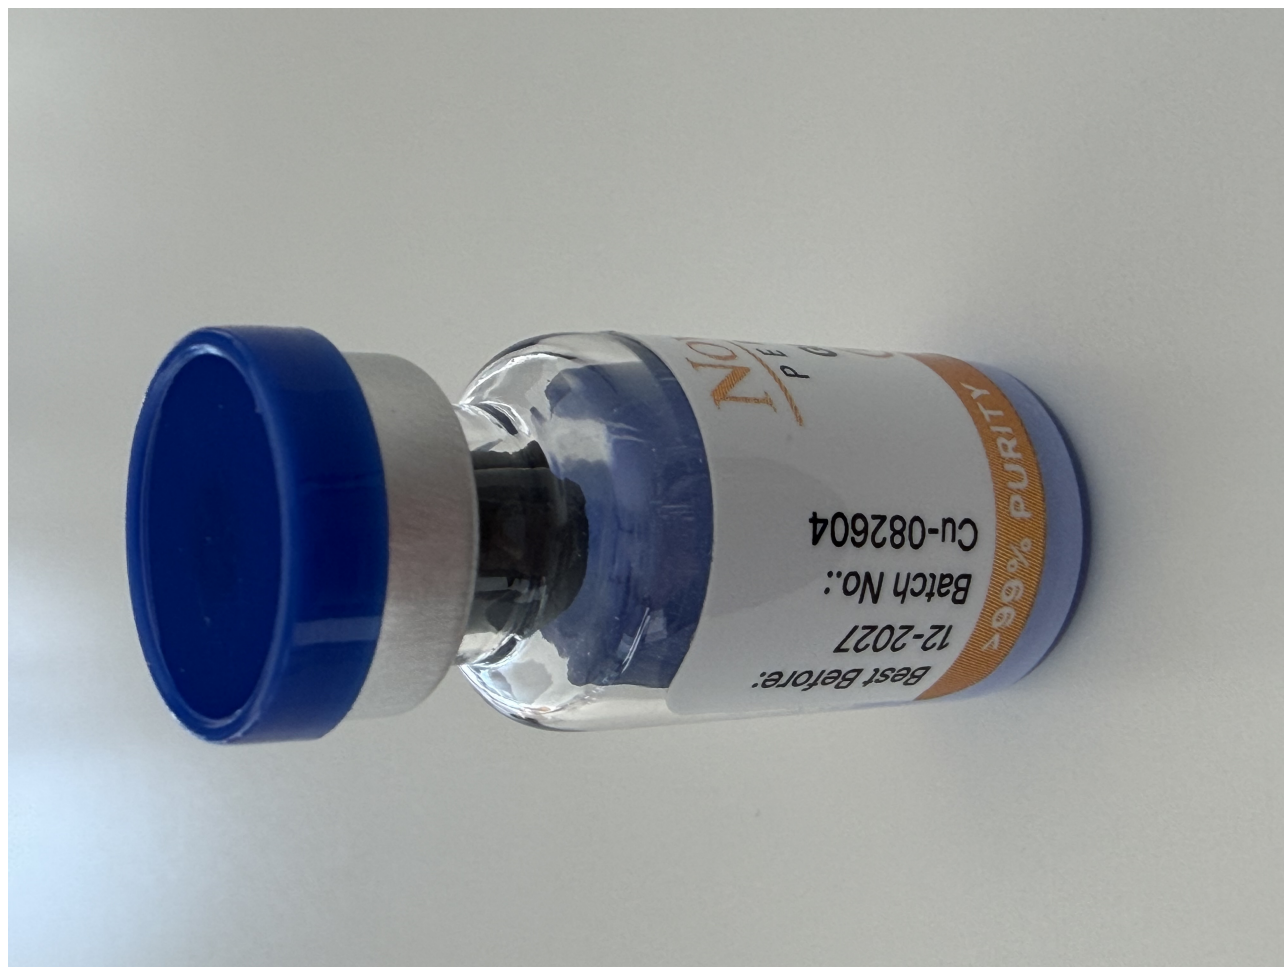

Endotoxin Determination Report




File Information

Filename: C:\UVVis-Data\Data\File_260923_142948.vqud
Date/Time: 09/23/2026 03:00:59 PM

Instrument Information

Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

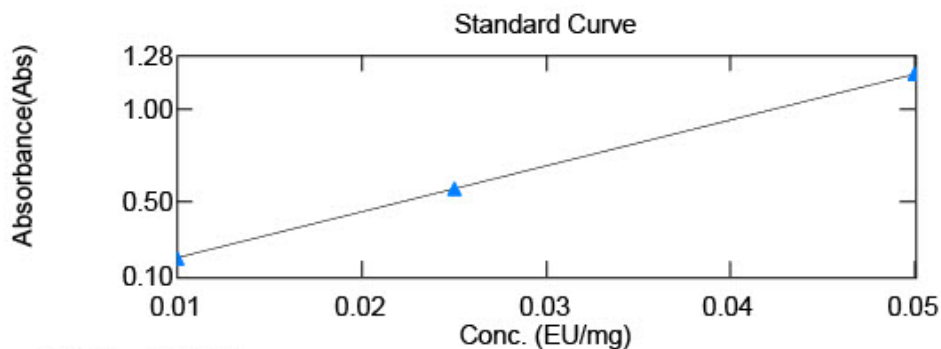

$$y = 24.7085x - 0.0501259$$
$$r^2 = 0.99999$$

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
1	LYO-0971	0.127	0.1067	20.00
2	LYO-0984	0.108	0.0831	20.00
3	LYO-0987	0.106	0.0802	20.00
4	LYO-0986	0.515	0.0771	100.00
5	LIQ-0075	0.021	0.4709	1.00
6	LIQ-0076	0.008	0.1574	1.00
7	LYO-0924	1.502	0.8775	40.00
8	LYO-0925	1.706	1.0039	40.00
9	LYO-0924 spike	2.070	1.2285	40.00
10	LYO-0925 spike	2.177	1.2945	40.00

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.